

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 01569
Calib. Date: 01/08/2015
Calib. No.: 00029
Certification File No.: 01570
Cert. Date: 01/08/2015
Cert. No.: 00022
Linearity File No.: 01571
Lin. Date: 01/08/2015
Lin. No.: 00022
Solution File No.: 01572
Soln. Date: 01/08/2015
Soln. No.: 00188
Sequential File No.: 01572
File Date: 01/08/2015

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 14A126
Model No.: CU-34
Serial No.: DDUF S3-0064
Expires: 01/06/2016
Bottle No.: 0541

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:15S		
Control 1 EC	0.101%	15:16S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:16S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:17S		
Control 2 EC	0.100%	15:17S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:17S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:18S		
Control 3 EC	0.100%	15:19S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:19S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:19S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with
Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DD5FP2 - 0396 (Ma)

Changed By:

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: Sgt. Michelle Goncalves #6040

Badge No.: 6040

Date: 01/08/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01569 Calib. Date: 01/08/2015 Calib. No.: 00029
Certification File No.: 01570 Cert. Date: 01/08/2015 Cert. No.: 00022
Linearity File No.: 01571 Lin. Date: 01/08/2015 Lin. No.: 00022
Solution File No.: 01580 Soln. Date: 02/04/2015 Soln. No.: 00189
Sequential File No.: 01580 File Date: 02/04/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 01/06/2016
Solution Control Lot: 14A126 Bottle No.: 0537

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:55S		
Control 1 EC	0.101%	16:56S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:56S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:57S		
Control 2 EC	0.100%	16:57S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:57S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:58S		
Control 3 EC	0.099%	16:59S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	16:59S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:00S		

All tests within acceptable tolerance.

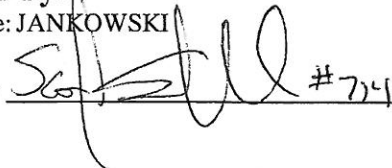
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 02/04/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01569 Calib. Date: 01/08/2015 Calib. No.: 00029
Certification File No.: 01570 Cert. Date: 01/08/2015 Cert. No.: 00022
Linearity File No.: 01571 Lin. Date: 01/08/2015 Lin. No.: 00022
Solution File No.: 01586 Soln. Date: 02/28/2015 Soln. No.: 00190
Sequential File No.: 01586 File Date: 02/28/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 01/06/2016
Solution Control Lot: 14A126 Bottle No.: 0542

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:27S		
Control 1 EC	0.100%	13:28S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:28S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:28S		
Control 2 EC	0.097%	13:29S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:29S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:30S		
Control 3 EC	0.097%	13:31S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	13:31S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:31S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 02/28/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01569 **Calib. Date:** 01/08/2015 **Calib. No.:** 00029
Certification File No.: 01570 **Cert. Date:** 01/08/2015 **Cert. No.:** 00022
Linearity File No.: 01571 **Lin. Date:** 01/08/2015 **Lin. No.:** 00022
Solution File No.: 01592 **Soln. Date:** 04/09/2015 **Soln. No.:** 00192
Sequential File No.: 01592 **File Date:** 04/09/2015

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 01/06/2016
Solution Control Lot: 14A126 **Bottle No.:** 0539

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:35D		
Control 1 EC	-.---%	14:35D	23.9°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	14:35D	23.9°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

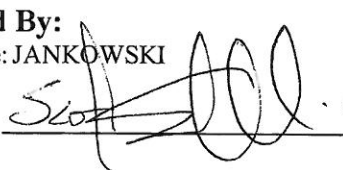
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 04/09/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01569 Calib. Date: 01/08/2015 Calib. No.: 00029
Certification File No.: 01570 Cert. Date: 01/08/2015 Cert. No.: 00022
Linearity File No.: 01571 Lin. Date: 01/08/2015 Lin. No.: 00022
Solution File No.: 01593 Soln. Date: 04/09/2015 Soln. No.: 00193
Sequential File No.: 01593 File Date: 04/09/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 01/06/2016
Solution Control Lot: 14A126 Bottle No.: 0538

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:07D		
Control 1 EC	0.101%	16:07D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:07D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:08D		
Control 2 EC	0.099%	16:09D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	16:09D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:10D		
Control 3 EC	0.099%	16:10D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	16:10D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  # 714

Badge No.: 714

Date: 04/09/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01569 Calib. Date: 01/08/2015 Calib. No.: 00029
Certification File No.: 01570 Cert. Date: 01/08/2015 Cert. No.: 00022
Linearity File No.: 01571 Lin. Date: 01/08/2015 Lin. No.: 00022
Solution File No.: 01608 Soln. Date: 05/11/2015 Soln. No.: 00194
Sequential File No.: 01608 File Date: 05/11/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 01/06/2016
Solution Control Lot: 14A126 Bottle No.: 0540

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:07D		
Control 1 EC	0.100%	13:07D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:07D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:08D		
Control 2 EC	0.099%	13:09D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:09D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:09D		
Control 3 EC	0.099%	13:10D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:10D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  # 714

Badge No.: 714

Date: 05/11/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01569 Calib. Date: 01/08/2015 Calib. No.: 00029
Certification File No.: 01570 Cert. Date: 01/08/2015 Cert. No.: 00022
Linearity File No.: 01571 Lin. Date: 01/08/2015 Lin. No.: 00022
Solution File No.: 01612 Soln. Date: 06/01/2015 Soln. No.: 00195
Sequential File No.: 01612 File Date: 06/01/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 01/06/2016
Solution Control Lot: 14A126 Bottle No.: 0543

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:13D		
Control 1 EC	0.100%	13:13D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:13D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:14D		
Control 2 EC	0.099%	13:14D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:15D		
Control 3 EC	0.100%	13:16D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:16D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:16D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature: 

Badge No.: 714

Date: 06/01/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01569 **Calib. Date:** 01/08/2015 **Calib. No.:** 00029
Certification File No.: 01570 **Cert. Date:** 01/08/2015 **Cert. No.:** 00022
Linearity File No.: 01571 **Lin. Date:** 01/08/2015 **Lin. No.:** 00022
Solution File No.: 01621 **Soln. Date:** 06/29/2015 **Soln. No.:** 00196
Sequential File No.: 01621 **File Date:** 06/29/2015

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 01/06/2016
Solution Control Lot: 14A126 **Bottle No.:** 0544

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:52D		
Control 1 EC	0.100%	14:52D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:52D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:53D		
Control 2 EC	0.099%	14:53D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:53D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:54D		
Control 3 EC	0.099%	14:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	14:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:55D		

All tests within acceptable tolerance.

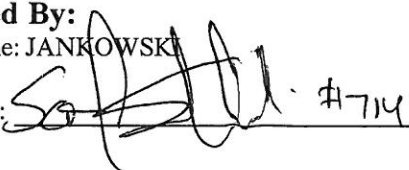
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 06/29/2015

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 01622 Calib. Date: 07/06/2015 Calib. No.: 00030
Certification File No.: 01623 Cert. Date: 07/06/2015 Cert. No.: 00023
Linearity File No.: 01624 Lin. Date: 07/06/2015 Lin. No.: 00023
Solution File No.: 01625 Soln. Date: 07/06/2015 Soln. No.: 00197
Sequential File No.: 01625 File Date: 07/06/2015

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 14A126

Model No.: CU-34

Serial No.: DDUF S3-0064
Expires: 01/06/2016
Bottle No.: 0545

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:21D		
Control 1 EC	0.102%	12:22D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	12:22D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:23D		
Control 2 EC	0.102%	12:23D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:23D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:24D		
Control 3 EC	0.101%	12:24D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	12:24D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:25D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with
Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDSF P2 - 0396 (MGA)

Changed By:

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: Sgt. Michelle Goncalves #6040

Badge No.: 6040

Date: 07/06/2015

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 01622
Calib. Date: 07/06/2015
Calib. No.: 00030
Certification File No.: 01623
Cert. Date: 07/06/2015
Cert. No.: 00023
Linearity File No.: 01624
Lin. Date: 07/06/2015
Lin. No.: 00023
Solution File No.: 01634
Soln. Date: 08/14/2015
Soln. No.: 00198
Sequential File No.: 01634
File Date: 08/14/2015

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 14A126
Model No.: CU-34
Serial No.: DDUF S3-0064
Expires: 01/06/2016
Bottle No.: 0546

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:26D		
Control 1 EC	0.101%	18:27D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	18:27D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:27D		
Control 2 EC	0.101%	18:28D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	18:28D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:28D		
Control 3 EC	0.101%	18:29D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	18:29D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:30D		

All tests within acceptable tolerance.

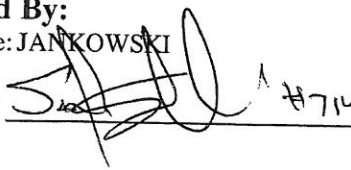
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature: 

Badge No.: 714

Date: 08/14/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01622 **Calib. Date:** 07/06/2015 **Calib. No.:** 00030
Certification File No.: 01623 **Cert. Date:** 07/06/2015 **Cert. No.:** 00023
Linearity File No.: 01624 **Lin. Date:** 07/06/2015 **Lin. No.:** 00023
Solution File No.: 01645 **Soln. Date:** 09/16/2015 **Soln. No.:** 00199
Sequential File No.: 01645 **File Date:** 09/16/2015

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 01/06/2016
Solution Control Lot: 14A126 **Bottle No.:** 0547

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:36D		
Control 1 EC	0.101%	12:36D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	12:36D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:37D		
Control 2 EC	0.101%	12:37D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	12:37D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:38D		
Control 3 EC	0.101%	12:39D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:39D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 09/16/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01622 **Calib. Date:** 07/06/2015 **Calib. No.:** 00030
Certification File No.: 01623 **Cert. Date:** 07/06/2015 **Cert. No.:** 00023
Linearity File No.: 01624 **Lin. Date:** 07/06/2015 **Lin. No.:** 00023
Solution File No.: 01656 **Soln. Date:** 10/08/2015 **Soln. No.:** 00200
Sequential File No.: 01656 **File Date:** 10/08/2015

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 01/06/2016
Solution Control Lot: 14A126 **Bottle No.:** 0548

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:21D		
Control 1 EC	0.102%	15:21D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	15:21D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:22D		
Control 2 EC	0.101%	15:23D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	15:23D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:23D		
Control 3 EC	0.101%	15:24D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	15:24D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:25D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: _____

Sgt. Michelle Goncalves #6040

Badge No.: 6040

Date: 10/08/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01622 Calib. Date: 07/06/2015 Calib. No.: 00030
Certification File No.: 01623 Cert. Date: 07/06/2015 Cert. No.: 00023
Linearity File No.: 01624 Lin. Date: 07/06/2015 Lin. No.: 00023
Solution File No.: 01666 Soln. Date: 11/07/2015 Soln. No.: 00201
Sequential File No.: 01666 File Date: 11/07/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 01/06/2016
Solution Control Lot: 14A126 Bottle No.: 0549

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:10S		
Control 1 EC	0.099%	18:11S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:11S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:12S		
Control 2 EC	0.099%	18:12S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:12S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:13S		
Control 3 EC	0.099%	18:13S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	18:13S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:14S		

All tests within acceptable tolerance.

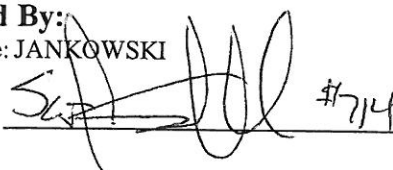
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature: 

Badge No.: 714

Date: 11/07/2015

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 01683
Calib. Date: 12/07/2015
Calib. No.: 00031
Certification File No.: 01684
Cert. Date: 12/07/2015
Cert. No.: 00024
Linearity File No.: 01685
Lin. Date: 12/07/2015
Lin. No.: 00024
Solution File No.: 01686
Soln. Date: 12/07/2015
Soln. No.: 00202
Sequential File No.: 01686
File Date: 12/07/2015

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 15H140
Model No.: CU-34
Serial No.: DDUF S3-0065
Expires: 08/04/2017
Bottle No.: 0762

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:03S		
Control 1 EC	0.101%	12:04S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	12:04S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:04S		
Control 2 EC	0.100%	12:05S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:05S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:06S		
Control 3 EC	0.100%	12:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number:

DDUJP2-144

(MA)

Changed By:

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature:

Sgt. Michelle Goncalves #6040

Badge No.: 6040

Date: 12/07/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01683 **Calib. Date:** 12/07/2015 **Calib. No.:** 00031
Certification File No.: 01684 **Cert. Date:** 12/07/2015 **Cert. No.:** 00024
Linearity File No.: 01685 **Lin. Date:** 12/07/2015 **Lin. No.:** 00024
Solution File No.: 01696 **Soln. Date:** 12/20/2015 **Soln. No.:** 00203
Sequential File No.: 01696 **File Date:** 12/20/2015

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0065
Control Solution %: 0.100% **Expires:** 08/04/2017
Solution Control Lot: 15H140 **Bottle No.:** 0766

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:11S		
Control 1 EC	0.100%	14:12S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:12S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:13S		
Control 2 EC	0.099%	14:13S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:13S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:14S		
Control 3 EC	0.099%	14:15S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:15S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:15S		

All tests within acceptable tolerance.

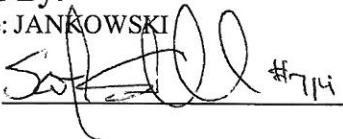
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 12/20/2015