

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00403 Calib. Date: 11/14/2007 Calib. No.: 00007
Certification File No.: 00404 Cert. Date: 11/14/2007 Cert. No.: 00005
Linearity File No.: 00405 Lin. Date: 11/14/2007 Lin. No.: 00005
Solution File No.: 00432 Soln. Date: 01/07/2008 Soln. No.: 00061
Sequential File No.: 00432 File Date: 01/07/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 11/17/2008
Solution Control Lot: 06K037 Bottle No.: 0711

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	22:28S		
Control 1 EC	0.100%	22:28S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	22:28S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:29S		
Control 2 EC	0.098%	22:30S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	22:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:30S		
Control 3 EC	0.099%	22:31S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	22:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:32S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BRESNEN

First Name: JOHN

MI: A

Signature:



Badge No.: 531

Date: 01/07/2008

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 00403
Calib. Date: 11/14/2007
Calib. No.: 00007
Certification File No.: 00404
Cert. Date: 11/14/2007
Cert. No.: 00005
Linearity File No.: 00405
Lin. Date: 11/14/2007
Lin. No.: 00005
Solution File No.: 00445
Soln. Date: 02/06/2008
Soln. No.: 00062
Sequential File No.: 00445
File Date: 02/06/2008

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 06K037
Model No.: CU-34
Serial No.: DDUF S3-0064
Expires: 11/17/2008
Bottle No.: 0712

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:48S		
Control 1 EC	0.100%	09:48S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:49S		
Control 2 EC	0.098%	09:50S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:51S		
Control 3 EC	0.099%	09:51S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:52S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with
Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDSFP2-0396 *(Signature)*

Changed By:

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: *TPR II Thomas J. Snyder #5792*

Badge No.: 5792

Date: 02/06/2008

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 00403
Calib. Date: 11/14/2007
Calib. No.: 00007
Certification File No.: 00404
Cert. Date: 11/14/2007
Cert. No.: 00005
Linearity File No.: 00405
Lin. Date: 11/14/2007
Lin. No.: 00005
Solution File No.: 00451
Soln. Date: 03/04/2008
Soln. No.: 00063
Sequential File No.: 00451
File Date: 03/04/2008

Calibrating Unit: WET
Model No.: CU-34
Serial No.: DDUF S3-0064
Control Solution %: 0.100%
Expires: 11/17/2008
Solution Control Lot: 06K037
Bottle No.: 0713

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:56S		
Control 1 EC	0.100%	17:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	17:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:57S		
Control 2 EC	0.098%	17:58S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	17:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:59S		
Control 3 EC	0.099%	17:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	17:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:00S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 03/04/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00403 Calib. Date: 11/14/2007 Calib. No.: 00007
Certification File No.: 00404 Cert. Date: 11/14/2007 Cert. No.: 00005
Linearity File No.: 00405 Lin. Date: 11/14/2007 Lin. No.: 00005
Solution File No.: 00457 Soln. Date: 04/01/2008 Soln. No.: 00064
Sequential File No.: 00457 File Date: 04/01/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 11/17/2008
Solution Control Lot: 06K037 Bottle No.: 0714

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:44S		
Control 1 EC	0.101%	09:45S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:45S		
Control 2 EC	0.098%	09:46S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:47S		
Control 3 EC	0.099%	09:47S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:48S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 04/01/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0005
Location:	PLAINSBORO TOWNSHIP PD		
Calibration File No.:	00403	Calib. Date:	11/14/2007
Certification File No.:	00404	Cert. Date:	11/14/2007
Linearity File No.:	00405	Lin. Date:	11/14/2007
Solution File No.:	00465	Soln. Date:	04/30/2008
Sequential File No.:	00465	File Date:	04/30/2008
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUF S3-0064
Solution Control Lot:	06K037	Expires:	11/17/2008
		Bottle No.:	0715

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:28D		
Control 1 EC	0.098%	15:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:30D		
Control 2 EC	0.097%	15:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:31D		
Control 3 EC	0.098%	15:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	15:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:32D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 04/30/2008

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 00403
Calib. Date: 11/14/2007
Calib. No.: 00007
Certification File No.: 00404
Cert. Date: 11/14/2007
Cert. No.: 00005
Linearity File No.: 00405
Lin. Date: 11/14/2007
Lin. No.: 00005
Solution File No.: 00476
Soln. Date: 05/24/2008
Soln. No.: 00066
Sequential File No.: 00476
File Date: 05/24/2008

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 06K037
Model No.: CU-34
Serial No.: DDUF S3-0064
Expires: 11/17/2008
Bottle No.: 0716

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:28D		
Control 1 EC	0.098%	15:28D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	15:28D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:29D		
Control 2 EC	0.097%	15:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	15:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:30D		
Control 3 EC	0.097%	15:31D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	15:31D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:32D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BRESNEN

First Name: JOHN

MI: A

Signature:



Badge No.: 531

Date: 05/24/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00403 Calib. Date: 11/14/2007 Calib. No.: 00007
Certification File No.: 00404 Cert. Date: 11/14/2007 Cert. No.: 00005
Linearity File No.: 00405 Lin. Date: 11/14/2007 Lin. No.: 00005
Solution File No.: 00485 Soln. Date: 06/19/2008 Soln. No.: 00067
Sequential File No.: 00485 File Date: 06/19/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 11/17/2008
Solution Control Lot: 06K037 Bottle No.: 0717

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:32D		
Control 1 EC	0.099%	08:32D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:33D		
Control 2 EC	0.098%	08:33D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:34D		
Control 3 EC	0.099%	08:35D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	08:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:35D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 06/19/2008

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 00403
Calib. Date: 11/14/2007
Calib. No.: 00007
Certification File No.: 00404
Cert. Date: 11/14/2007
Cert. No.: 00005
Linearity File No.: 00405
Lin. Date: 11/14/2007
Lin. No.: 00005
Solution File No.: 00492
Soln. Date: 07/20/2008
Soln. No.: 00068
Sequential File No.: 00492
File Date: 07/20/2008

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 06K037
Model No.: CU-34
Serial No.: DDUF S3-0064
Expires: 11/17/2008
Bottle No.: 0718

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:05D		
Control 1 EC	0.100%	19:05D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	19:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:06D		
Control 2 EC	0.098%	19:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	19:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:07D		
Control 3 EC	0.098%	19:08D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	19:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 07/20/2008

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 00497
Calib. Date: 07/28/2008
Calib. No.: 00008
Certification File No.: 00498
Cert. Date: 07/28/2008
Cert. No.: 00006
Linearity File No.: 00499
Lin. Date: 07/28/2008
Lin. No.: 00006
Solution File No.: 00508
Soln. Date: 08/18/2008
Soln. No.: 00070
Sequential File No.: 00508
File Date: 08/18/2008

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 06K037
Model No.: CU-34
Serial No.: DDUF S3-0065
Expires: 11/17/2008
Bottle No.: 0719

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:29D		
Control 1 EC	0.099%	16:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	16:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:30D		
Control 2 EC	0.098%	16:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:31D		
Control 3 EC	0.099%	16:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	16:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:33D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  # 714

Badge No.: 714

Date: 08/18/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00497 Calib. Date: 07/28/2008 Calib. No.: 00008
Certification File No.: 00498 Cert. Date: 07/28/2008 Cert. No.: 00006
Linearity File No.: 00499 Lin. Date: 07/28/2008 Lin. No.: 00006
Solution File No.: 00517 Soln. Date: 09/16/2008 Soln. No.: 00071
Sequential File No.: 00517 File Date: 09/16/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 11/17/2008
Solution Control Lot: 06K037 Bottle No.: 0720

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:36D		
Control 1 EC	0.099%	19:36D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	19:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:37D		
Control 2 EC	0.098%	19:37D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	19:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:38D		
Control 3 EC	0.099%	19:39D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	19:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:39D		

All tests within acceptable tolerance.

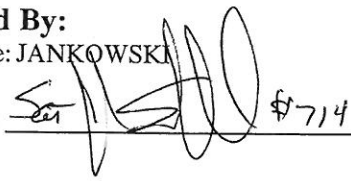
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  714

Badge No.: 714

Date: 09/16/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0005
Location:	PLAINSBORO TOWNSHIP PD		
Calibration File No.:	00497	Calib. Date:	07/28/2008
Certification File No.:	00498	Cert. No.:	00006
Linearity File No.:	00499	Lin. Date:	07/28/2008
Solution File No.:	00530	Soln. No.:	00072
Sequential File No.:	00530	File Date:	10/10/2008
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUF S3-0065
Solution Control Lot:	06K037	Expires:	11/17/2008
		Bottle No.:	0721

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:51D		
Control 1 EC	0.099%	08:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:53D		
Control 2 EC	0.098%	08:53D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:54D		
Control 3 EC	0.098%	08:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	08:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:55D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 10/10/2008

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 00497
Calib. Date: 07/28/2008
Calib. No.: 00008
Certification File No.: 00498
Cert. Date: 07/28/2008
Cert. No.: 00006
Linearity File No.: 00499
Lin. Date: 07/28/2008
Lin. No.: 00006
Solution File No.: 00538
Soln. Date: 11/07/2008
Soln. No.: 00073
Sequential File No.: 00538
File Date: 11/07/2008

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 08G058
Model No.: CU-34
Serial No.: DDUF S3-0065
Expires: 07/23/2010
Bottle No.: 0901

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:14S		
Control 1 EC	0.099%	15:15S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:16S		
Control 2 EC	0.097%	15:16S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:17S		
Control 3 EC	0.097%	15:18S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	15:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:18S		

All tests within acceptable tolerance.

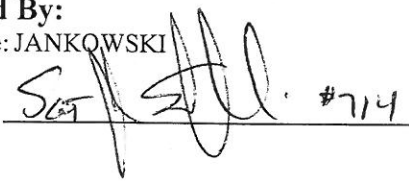
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 11/07/2008

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 00497
Calib. Date: 07/28/2008
Calib. No.: 00008
Certification File No.: 00498
Cert. Date: 07/28/2008
Cert. No.: 00006
Linearity File No.: 00499
Lin. Date: 07/28/2008
Lin. No.: 00006
Solution File No.: 00547
Soln. Date: 11/25/2008
Soln. No.: 00074
Sequential File No.: 00547
File Date: 11/25/2008

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 08G058
Model No.: CU-34
Serial No.: DDUF S3-0065
Expires: 07/23/2010
Bottle No.: 0902

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:36S		
Control 1 EC	0.100%	07:37S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	07:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:38S		
Control 2 EC	0.098%	07:38S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	07:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:39S		
Control 3 EC	0.099%	07:40S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	07:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:40S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 11/25/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00497 Calib. Date: 07/28/2008 Calib. No.: 00008
Certification File No.: 00498 Cert. Date: 07/28/2008 Cert. No.: 00006
Linearity File No.: 00499 Lin. Date: 07/28/2008 Lin. No.: 00006
Solution File No.: 00558 Soln. Date: 12/17/2008 Soln. No.: 00075
Sequential File No.: 00558 File Date: 12/17/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 07/23/2010
Solution Control Lot: 08G058 Bottle No.: 0903

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:12S		
Control 1 EC	0.099%	13:13S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:14S		
Control 2 EC	0.097%	13:14S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:15S		
Control 3 EC	0.098%	13:16S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:16S		

All tests within acceptable tolerance.

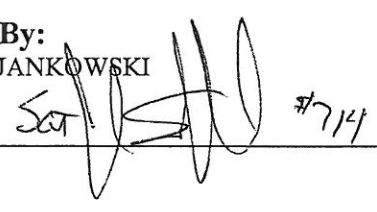
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature: 

Badge No.: 714

Date: 12/17/2008