

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0005
Location:	PLAINSBORO TOWNSHIP PD	
Calibration File No.:	00497	Calib. No.: 00008
Certification File No.:	00498	Cert. No.: 00006
Linearity File No.:	00499	Lin. No.: 00006
Solution File No.:	00571	Soln. No.: 00076
Sequential File No.:	00571	File Date: 01/08/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUF S3-0065
Solution Control Lot:	08G058	Expires: 07/23/2010
		Bottle No.: 0904

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:33S		
Control 1 EC	0.100%	15:33S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:34S		
Control 2 EC	0.098%	15:35S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:36S		
Control 3 EC	0.099%	15:36S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:37S		

All tests within acceptable tolerance.

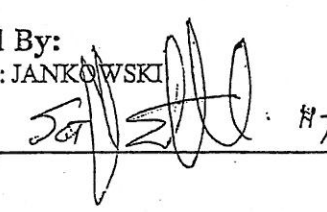
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 01/08/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00578 **Calib. Date:** 01/20/2009 **Calib. No.:** 00009
Certification File No.: 00579 **Cert. Date:** 01/20/2009 **Cert. No.:** 00007
Linearity File No.: 00580 **Lin. Date:** 01/20/2009 **Lin. No.:** 00007
Solution File No.: 00587 **Soln. Date:** 02/01/2009 **Soln. No.:** 00078
Sequential File No.: 00587 **File Date:** 02/01/2009

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 07/23/2010
Solution Control Lot: 08G058 **Bottle No.:** 0905

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:20S		
Control 1 EC	0.100%	12:21S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:22S		
Control 2 EC	0.097%	12:22S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:23S		
Control 3 EC	0.098%	12:24S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:25S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature: 

Badge No.: 714

Date: 02/01/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00578 Calib. Date: 01/20/2009 Calib. No.: 00009
Certification File No.: 00579 Cert. Date: 01/20/2009 Cert. No.: 00007
Linearity File No.: 00580 Lin. Date: 01/20/2009 Lin. No.: 00007
Solution File No.: 00593 Soln. Date: 02/19/2009 Soln. No.: 00079
Sequential File No.: 00593 File Date: 02/19/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 07/23/2010
Solution Control Lot: 08G058 Bottle No.: 0907

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:11S		
Control 1 EC	0.099%	15:12S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:12S		
Control 2 EC	0.097%	15:13S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:14S		
Control 3 EC	0.098%	15:14S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	15:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:15S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature: 

Badge No.: 714

Date: 02/19/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00578 **Calib. Date:** 01/20/2009 **Calib. No.:** 00009
Certification File No.: 00579 **Cert. Date:** 01/20/2009 **Cert. No.:** 00007
Linearity File No.: 00580 **Lin. Date:** 01/20/2009 **Lin. No.:** 00007
Solution File No.: 00602 **Soln. Date:** 03/18/2009 **Soln. No.:** 00080
Sequential File No.: 00602 **File Date:** 03/18/2009

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 07/23/2010
Solution Control Lot: 08G058 **Bottle No.:** 0908

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:21S		
Control 1 EC	0.100%	15:22S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:23S		
Control 2 EC	0.099%	15:23S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	15:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:24S		
Control 3 EC	0.098%	15:25S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	15:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:26S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 03/18/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0005
Location:	PLAINSBORO TOWNSHIP PD		
Calibration File No.:	00578	Calib. Date:	01/20/2009
Certification File No.:	00579	Cert. Date:	01/20/2009
Linearity File No.:	00580	Lin. Date:	01/20/2009
Solution File No.:	00609	Soln. Date:	04/19/2009
Sequential File No.:	00609	File Date:	04/19/2009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUF S3-0064
Solution Control Lot:	08G058	Expires:	07/23/2010
		Bottle No.:	0909

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:17D		
Control 1 EC	0.100%	15:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:18D		
Control 2 EC	0.098%	15:19D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	15:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:20D		
Control 3 EC	0.099%	15:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	15:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:21D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BRESNEN

First Name: JOHN

MI: A

Signature:

John J. Bresnen #531

Badge No.: 531

Date: 04/19/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00578 Calib. Date: 01/20/2009 Calib. No.: 00009
Certification File No.: 00579 Cert. Date: 01/20/2009 Cert. No.: 00007
Linearity File No.: 00580 Lin. Date: 01/20/2009 Lin. No.: 00007
Solution File No.: 00621 Soln. Date: 05/22/2009 Soln. No.: 00082
Sequential File No.: 00621 File Date: 05/22/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 07/23/2010
Solution Control Lot: 08G058 Bottle No.: 0910

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:51D		
Control 1 EC	0.099%	08:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:53D		
Control 2 EC	0.098%	08:53D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:54D		
Control 3 EC	0.099%	08:54D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:55D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 05/22/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00578 Calib. Date: 01/20/2009 Calib. No.: 00009
Certification File No.: 00579 Cert. Date: 01/20/2009 Cert. No.: 00007
Linearity File No.: 00580 Lin. Date: 01/20/2009 Lin. No.: 00007
Solution File No.: 00626 Soln. Date: 06/20/2009 Soln. No.: 00083
Sequential File No.: 00626 File Date: 06/20/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 07/23/2010
Solution Control Lot: 08G058 Bottle No.: 0911

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:12D		
Control 1 EC	0.099%	15:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:13D		
Control 2 EC	0.098%	15:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:14D		
Control 3 EC	0.099%	15:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	15:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:16D		

All tests within acceptable tolerance.

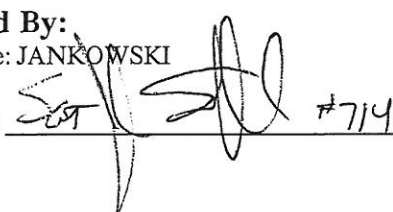
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 06/20/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00634 **Calib. Date:** 07/06/2009 **Calib. No.:** 00010
Certification File No.: 00635 **Cert. Date:** 07/06/2009 **Cert. No.:** 00008
Linearity File No.: 00636 **Lin. Date:** 07/06/2009 **Lin. No.:** 00008
Solution File No.: 00637 **Soln. Date:** 07/06/2009 **Soln. No.:** 00084
Sequential File No.: 00637 **File Date:** 07/06/2009

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 07/23/2010
Solution Control Lot: 08G058 **Bottle No.:** 0912

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:41D		
Control 1 EC	0.100%	16:42D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	16:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:43D		
Control 2 EC	0.099%	16:43D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	16:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:44D		
Control 3 EC	0.099%	16:44D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	16:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:45D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: MSFP2 - 0396

(Signature)

Changed By:

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: *TH. J. Snyder #5792*

Badge No.: 5792

Date: 07/06/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00634 **Calib. Date:** 07/06/2009 **Calib. No.:** 00010
Certification File No.: 00635 **Cert. Date:** 07/06/2009 **Cert. No.:** 00008
Linearity File No.: 00636 **Lin. Date:** 07/06/2009 **Lin. No.:** 00008
Solution File No.: 00648 **Soln. Date:** 07/30/2009 **Soln. No.:** 00085
Sequential File No.: 00648 **File Date:** 07/30/2009

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 07/23/2010
Solution Control Lot: 08G058 **Bottle No.:** 0913

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:17D		
Control 1 EC	0.099%	12:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	12:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:18D		
Control 2 EC	0.098%	12:19D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:19D		
Control 3 EC	0.098%	12:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	12:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:21D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature: SA JANKOWSKI #714

Badge No.: 714

Date: 07/30/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00634 Calib. Date: 07/06/2009 Calib. No.: 00010
Certification File No.: 00635 Cert. Date: 07/06/2009 Cert. No.: 00008
Linearity File No.: 00636 Lin. Date: 07/06/2009 Lin. No.: 00008
Solution File No.: 00657 Soln. Date: 08/19/2009 Soln. No.: 00086
Sequential File No.: 00657 File Date: 08/19/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 07/23/2010
Solution Control Lot: 08G058 Bottle No.: 0914

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:37D		
Control 1 EC	0.098%	14:37D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:38D		
Control 2 EC	0.097%	14:39D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:39D		
Control 3 EC	0.098%	14:40D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	14:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:41D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature: 

Badge No.: 714

Date: 08/19/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00634 **Calib. Date:** 07/06/2009 **Calib. No.:** 00010
Certification File No.: 00635 **Cert. Date:** 07/06/2009 **Cert. No.:** 00008
Linearity File No.: 00636 **Lin. Date:** 07/06/2009 **Lin. No.:** 00008
Solution File No.: 00664 **Soln. Date:** 09/05/2009 **Soln. No.:** 00087
Sequential File No.: 00664 **File Date:** 09/05/2009

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 07/23/2010
Solution Control Lot: 08G058 **Bottle No.:** 0915

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:29D		
Control 1 EC	0.097%	17:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	17:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:30D		
Control 2 EC	0.096%	17:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	17:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:32D		
Control 3 EC	0.097%	17:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	17:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:33D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 09/05/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0005
Location:	PLAINSBORO TOWNSHIP PD		
Calibration File No.:	00634	Calib. Date:	07/06/2009
Certification File No.:	00635	Cert. Date:	07/06/2009
Linearity File No.:	00636	Lin. Date:	07/06/2009
Solution File No.:	00667	Soln. Date:	09/11/2009
Sequential File No.:	00667	File Date:	09/11/2009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUF S3-0064
Solution Control Lot:	08G058	Expires:	07/23/2010
		Bottle No.:	0916

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:15D		
Control 1 EC	0.098%	15:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:17D		
Control 2 EC	0.097%	15:17D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	15:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:18D		
Control 3 EC	0.097%	15:18D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	15:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BRESNEN

First Name: JOHN

MI: A

Signature: Sgt. J. Bresnen

Badge No.: 731

Date: 09/11/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00634 Calib. Date: 07/06/2009 Calib. No.: 00010
Certification File No.: 00635 Cert. Date: 07/06/2009 Cert. No.: 00008
Linearity File No.: 00636 Lin. Date: 07/06/2009 Lin. No.: 00008
Solution File No.: 00677 Soln. Date: 10/10/2009 Soln. No.: 00089
Sequential File No.: 00677 File Date: 10/10/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 07/23/2010
Solution Control Lot: 08G058 Bottle No.: 0917

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:12D		
Control 1 EC	0.098%	18:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	18:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:13D		
Control 2 EC	0.096%	18:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	18:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:14D		
Control 3 EC	0.097%	18:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	18:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:16D		

All tests within acceptable tolerance.

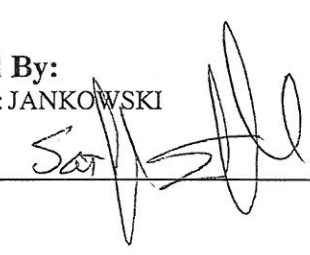
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 10/10/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00634 **Calib. Date:** 07/06/2009 **Calib. No.:** 00010
Certification File No.: 00635 **Cert. Date:** 07/06/2009 **Cert. No.:** 00008
Linearity File No.: 00636 **Lin. Date:** 07/06/2009 **Lin. No.:** 00008
Solution File No.: 00683 **Soln. Date:** 10/23/2009 **Soln. No.:** 00090
Sequential File No.: 00683 **File Date:** 10/23/2009

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 07/23/2010
Solution Control Lot: 08G058 **Bottle No.:** 0918

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:49D		
Control 1 EC	0.098%	18:49D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	18:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:50D		
Control 2 EC	0.097%	18:51D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	18:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:52D		
Control 3 EC	0.097%	18:52D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	18:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:53D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 10/23/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00634 Calib. Date: 07/06/2009 Calib. No.: 00010
Certification File No.: 00635 Cert. Date: 07/06/2009 Cert. No.: 00008
Linearity File No.: 00636 Lin. Date: 07/06/2009 Lin. No.: 00008
Solution File No.: 00689 Soln. Date: 10/30/2009 Soln. No.: 00091
Sequential File No.: 00689 File Date: 10/30/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 07/23/2010
Solution Control Lot: 08G058 Bottle No.: 0919

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:48S		
Control 1 EC	0.099%	23:49S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	23:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:50S		
Control 2 EC	0.097%	23:50S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	23:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:51S		
Control 3 EC	0.097%	23:52S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	23:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:52S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BRESNEN

First Name: JOHN

MI: A

Signature: Sgt. J. Bresnen #731

Badge No.: 731

Date: 10/30/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00634 Calib. Date: 07/06/2009 Calib. No.: 00010
Certification File No.: 00635 Cert. Date: 07/06/2009 Cert. No.: 00008
Linearity File No.: 00636 Lin. Date: 07/06/2009 Lin. No.: 00008
Solution File No.: 00700 Soln. Date: 11/20/2009 Soln. No.: 00092
Sequential File No.: 00700 File Date: 11/20/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 07/23/2010
Solution Control Lot: 08G058 Bottle No.: 0920

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:07S		
Control 1 EC	0.099%	18:08S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	18:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:08S		
Control 2 EC	0.098%	18:09S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	18:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:10S		
Control 3 EC	0.098%	18:10S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	18:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:11S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature: 

Badge No.: 714

Date: 11/20/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00706 **Calib. Date:** 12/10/2009 **Calib. No.:** 00013
Certification File No.: 00707 **Cert. Date:** 12/10/2009 **Cert. No.:** 00009
Linearity File No.: 00708 **Lin. Date:** 12/10/2009 **Lin. No.:** 00009
Solution File No.: 00709 **Soln. Date:** 12/10/2009 **Soln. No.:** 00094
Sequential File No.: 00709 **File Date:** 12/10/2009

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0065
Control Solution %: 0.100% **Expires:** 07/23/2010
Solution Control Lot: 08G058 **Bottle No.:** 0922

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:09S		
Control 1 EC	0.100%	11:10S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:10S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:10S		
Control 2 EC	0.100%	11:11S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:11S		
Control 3 EC	0.100%	11:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:12S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDUF P2 - 144

(Signature)

Changed By:

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: *TPR. I Thomas J. Snyder #5792*

Badge No.: 5792

Date: 12/10/2009