

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00879 Calib. Date: 11/22/2010 Calib. No.: 00015
Certification File No.: 00880 Cert. Date: 11/22/2010 Cert. No.: 00011
Linearity File No.: 00881 Lin. Date: 11/22/2010 Lin. No.: 00011
Solution File No.: 00911 Soln. Date: 01/16/2011 Soln. No.: 00114
Sequential File No.: 00911 File Date: 01/16/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 12/31/2011
Solution Control Lot: 09L072 Bottle No.: 0265

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:13S		
Control 1 EC	0.099%	12:14S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:15S		
Control 2 EC	0.097%	12:15S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:16S		
Control 3 EC	0.098%	12:17S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:18S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: Pr. Joseph Beni 543

Badge No.: 543

Date: 01/16/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0005
Location:	PLAINSBORO TOWNSHIP PD	
Calibration File No.:	00879	Calib. Date: 11/22/2010
Certification File No.:	00880	Calib. No.: 00015
Linearity File No.:	00881	Cert. Date: 11/22/2010
Solution File No.:	00917	Cert. No.: 00011
Sequential File No.:	00917	Lin. Date: 11/22/2010
		Lin. No.: 00011
		Soln. Date: 02/03/2011
		Soln. No.: 00115
		File Date: 02/03/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUF S3-0065
Solution Control Lot:	09L072	Expires: 12/31/2011
		Bottle No.: 0269

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:11S		
Control 1 EC	0.100%	14:12S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:13S		
Control 2 EC	0.098%	14:13S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	14:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:14S		
Control 3 EC	0.098%	14:15S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	14:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:15S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL # DDUF P2-144

Changed By:

Last Name: DENNIS

First Name: MARC

MI: W.

Signature: TPI. I [Signature] #5925

Badge No.: 5925

Date: 02/03/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00879 Calib. Date: 11/22/2010 Calib. No.: 00015
Certification File No.: 00880 Cert. Date: 11/22/2010 Cert. No.: 00011
Linearity File No.: 00881 Lin. Date: 11/22/2010 Lin. No.: 00011
Solution File No.: 00921 Soln. Date: 02/18/2011 Soln. No.: 00116
Sequential File No.: 00921 File Date: 02/18/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 12/31/2011
Solution Control Lot: 09L072 Bottle No.: 0266

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:49S		
Control 1 EC	0.099%	11:50S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:51S		
Control 2 EC	0.098%	11:51S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:52S		
Control 3 EC	0.098%	11:52S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:53S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: P+1 Joseph SML 543

Badge No.: 543

Date: 02/18/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00879 Calib. Date: 11/22/2010 Calib. No.: 00015
Certification File No.: 00880 Cert. Date: 11/22/2010 Cert. No.: 00011
Linearity File No.: 00881 Lin. Date: 11/22/2010 Lin. No.: 00011
Solution File No.: 00925 Soln. Date: 03/06/2011 Soln. No.: 00117
Sequential File No.: 00925 File Date: 03/06/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 12/31/2011
Solution Control Lot: 09L072 Bottle No.: 0267

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:31S		
Control 1 EC	0.098%	00:32S	34.0°C	AMBIENT AIR CHECK ERR
Control 1 IR	-.---%	00:32S	34.0°C	AMBIENT AIR CHECK ERR
Ambient Air Blank	-.---%	00:33S		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: TAVENER

First Name: FREDERICK

MI: W

Signature: _____

Badge No.: 730

Date: 03/06/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00879 Calib. Date: 11/22/2010 Calib. No.: 00015
Certification File No.: 00880 Cert. Date: 11/22/2010 Cert. No.: 00011
Linearity File No.: 00881 Lin. Date: 11/22/2010 Lin. No.: 00011
Solution File No.: 00926 Soln. Date: 03/07/2011 Soln. No.: 00118
Sequential File No.: 00926 File Date: 03/07/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 12/31/2011
Solution Control Lot: 09L072 Bottle No.: 0270

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:04S		
Control 1 EC	0.098%	10:05S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06S		
Control 2 EC	0.097%	10:06S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	10:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:07S		
Control 3 EC	0.098%	10:08S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:08S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: TAVENER

First Name: FREDERICK

MI: W

Signature: 

Badge No.: 730

Date: 03/07/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00879 **Calib. Date:** 11/22/2010 **Calib. No.:** 00015
Certification File No.: 00880 **Cert. Date:** 11/22/2010 **Cert. No.:** 00011
Linearity File No.: 00881 **Lin. Date:** 11/22/2010 **Lin. No.:** 00011
Solution File No.: 00933 **Soln. Date:** 03/28/2011 **Soln. No.:** 00119
Sequential File No.: 00933 **File Date:** 03/28/2011

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0065
Control Solution %: 0.100% **Expires:** 12/31/2011
Solution Control Lot: 09L072 **Bottle No.:** 0271

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:25S		
Control 1 EC	0.099%	09:25S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:26S		
Control 2 EC	0.097%	09:27S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:27S		
Control 3 EC	0.098%	09:28S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:29S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: PHI Joseph DELL BENI 543

Badge No.: 543

Date: 03/28/2011

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00879
Certification File No.: 00880
Linearity File No.: 00881
Solution File No.: 00939
Sequential File No.: 00939

Serial No.: ARTL-0005

Calib. Date: 11/22/2010
Cert. Date: 11/22/2010
Lin. Date: 11/22/2010
Soln. Date: 04/15/2011
File Date: 04/15/2011

Calib. No.: 00015
Cert. No.: 00011
Lin. No.: 00011
Soln. No.: 00120

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 09L072

Model No.: CU-34

Serial No.: DDUF S3-0065
Expires: 12/31/2011
Bottle No.: 0272

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:51D		
Control 1 EC	0.099%	11:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:52D		
Control 2 EC	0.097%	11:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:53D		
Control 3 EC	0.099%	11:54D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: P+1 Joseph 8ML 543

Badge No.: 543

Date: 04/15/2011

Calibrating Unit

New Standard Solution Report

Equipment: Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00953 Calib. Date: 05/19/2011 Calib. No.: 00018
Certification File No.: 00954 Cert. Date: 05/19/2011 Cert. No.: 00012
Linearity File No.: 00955 Lin. Date: 05/19/2011 Lin. No.: 00012
Solution File No.: 00956 Soln. Date: 05/19/2011 Soln. No.: 00125
Sequential File No.: 00956 File Date: 05/19/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 12/16/2012
Solution Control Lot: 10L084 Bottle No.: 0376

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:32D		
Control 1 EC	0.100%	13:33D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:33D		
Control 2 EC	0.100%	13:34D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:35D		
Control 3 EC	0.100%	13:35D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:36D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL # DDUF PC-03910

Changed By:

Last Name: DENNIS

First Name: MARC

MI: W.

Signature:

TAL. I [Signature] #5925

Badge No.: 5925

Date: 05/19/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00953 **Calib. Date:** 05/19/2011 **Calib. No.:** 00018
Certification File No.: 00954 **Cert. Date:** 05/19/2011 **Cert. No.:** 00012
Linearity File No.: 00955 **Lin. Date:** 05/19/2011 **Lin. No.:** 00012
Solution File No.: 00965 **Soln. Date:** 06/10/2011 **Soln. No.:** 00126
Sequential File No.: 00965 **File Date:** 06/10/2011

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 12/31/2011
Solution Control Lot: 09L072 **Bottle No.:** 0273

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:27D		
Control 1 EC	0.101%	15:28D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:28D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:29D		
Control 2 EC	0.100%	15:29D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:30D		
Control 3 EC	0.100%	15:30D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:31D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: Joseph Beni

573

Badge No.: 543

Date: 06/10/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00953 **Calib. Date:** 05/19/2011 **Calib. No.:** 00018
Certification File No.: 00954 **Cert. Date:** 05/19/2011 **Cert. No.:** 00012
Linearity File No.: 00955 **Lin. Date:** 05/19/2011 **Lin. No.:** 00012
Solution File No.: 00974 **Soln. Date:** 07/07/2011 **Soln. No.:** 00127
Sequential File No.: 00974 **File Date:** 07/07/2011

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 12/31/2011
Solution Control Lot: 09L072 **Bottle No.:** 0274

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:33D		
Control 1 EC	0.100%	09:34D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:35D		
Control 2 EC	0.099%	09:35D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:36D		
Control 3 EC	0.099%	09:36D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:37D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: P+1 Joseph Beni 543

Badge No.: 543

Date: 07/07/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00953 **Calib. Date:** 05/19/2011 **Calib. No.:** 00018
Certification File No.: 00954 **Cert. Date:** 05/19/2011 **Cert. No.:** 00012
Linearity File No.: 00955 **Lin. Date:** 05/19/2011 **Lin. No.:** 00012
Solution File No.: 00979 **Soln. Date:** 08/02/2011 **Soln. No.:** 00128
Sequential File No.: 00979 **File Date:** 08/02/2011

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 12/31/2011
Solution Control Lot: 09L072 **Bottle No.:** 0275

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:35D		
Control 1 EC	0.099%	14:35D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:36D		
Control 2 EC	0.099%	14:36D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:37D		
Control 3 EC	0.099%	14:38D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:38D		

All tests within acceptable tolerance.

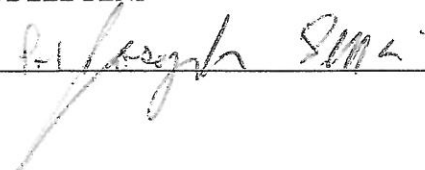
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: 

Badge No.: 543

Date: 08/02/2011

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00953
Certification File No.: 00954
Linearity File No.: 00955
Solution File No.: 00984
Sequential File No.: 00984

Serial No.: ARTL-0005

Calib. Date: 05/19/2011
Cert. Date: 05/19/2011
Lin. Date: 05/19/2011
Soln. Date: 08/19/2011
File Date: 08/19/2011

Calib. No.: 00018
Cert. No.: 00012
Lin. No.: 00012
Soln. No.: 00129

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 10L084

Model No.: CU-34

Serial No.: DDUF S3-0064
Expires: 12/16/2012
Bottle No.: 0377

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:03D		
Control 1 EC	0.100%	11:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:04D		
Control 2 EC	0.100%	11:05D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:05D		
Control 3 EC	0.100%	11:06D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: *Joseph Beni*

Badge No.: 543

Date: 08/19/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 00953 Calib. Date: 05/19/2011 Calib. No.: 00018
Certification File No.: 00954 Cert. Date: 05/19/2011 Cert. No.: 00012
Linearity File No.: 00955 Lin. Date: 05/19/2011 Lin. No.: 00012
Solution File No.: 00997 Soln. Date: 09/14/2011 Soln. No.: 00130
Sequential File No.: 00997 File Date: 09/14/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 12/16/2012
Solution Control Lot: 10L084 Bottle No.: 0378

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:39D		
Control 1 EC	0.100%	17:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	17:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:40D		
Control 2 EC	0.099%	17:40D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	17:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:41D		
Control 3 EC	0.100%	17:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:42D		

All tests within acceptable tolerance.

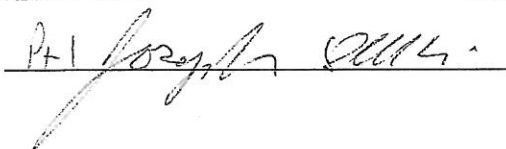
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: 

Badge No.: 543

Date: 09/14/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0005
Location:	PLAINSBORO TOWNSHIP PD		
Calibration File No.:	00953	Calib. Date:	05/19/2011
Certification File No.:	00954	Cert. Date:	05/19/2011
Linearity File No.:	00955	Lin. Date:	05/19/2011
Solution File No.:	01015	Soln. Date:	10/06/2011
Sequential File No.:	01015	File Date:	10/06/2011
		Calib. No.:	00018
		Cert. No.:	00012
		Lin. No.:	00012
		Soln. No.:	00131
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUF S3-0064
Solution Control Lot:	10L084	Expires:	12/16/2012
		Bottle No.:	0379

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:04D		
Control 1 EC	0.100%	16:05D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:05D		
Control 2 EC	0.100%	16:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	16:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:06D		
Control 3 EC	0.100%	16:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	16:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: P+1 Joseph L. 8004

Badge No.: 543

Date: 10/06/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0005
Location:	PLAINSBORO TOWNSHIP PD		
Calibration File No.:	00953	Calib. Date:	05/19/2011
Certification File No.:	00954	Cert. Date:	05/19/2011
Linearity File No.:	00955	Lin. Date:	05/19/2011
Solution File No.:	01034	Soln. Date:	10/28/2011
Sequential File No.:	01034	File Date:	10/28/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUF S3-0064
Solution Control Lot:	10L084	Expires:	12/16/2012
		Bottle No.:	0380

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:35D		
Control 1 EC	0.100%	20:36D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:36D		
Control 2 EC	0.100%	20:37D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:37D		
Control 3 EC	0.100%	20:38D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:39D		

All tests within acceptable tolerance.

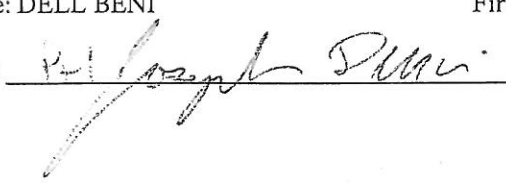
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: 

Badge No.: 543

Date: 10/28/2011

Calibrating Unit

New Standard Solution Report

Equipment: Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01042
Certification File No.: 01043
Linearity File No.: 01044
Solution File No.: 01045
Sequential File No.: 01045

Calib. Date: 11/16/2011
Cert. Date: 11/16/2011
Lin. Date: 11/16/2011
Soln. Date: 11/16/2011
File Date: 11/16/2011

Serial No.: ARTL-0005
Calib. No.: 00019
Cert. No.: 00013
Lin. No.: 00013
Soln. No.: 00133

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 10L084

Model No.: CU-34
Serial No.: DDUF S3-0065
Expires: 12/16/2012
Bottle No.: 0381

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:55S		
Control 1 EC	0.101%	11:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:56S		
Control 2 EC	0.101%	11:57S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:57S		
Control 3 EC	0.101%	11:58S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:59S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDUIP2-144 MPH

Changed By:

Last Name: GIBSON

First Name: MICHAEL

MI: P.

Signature:

Tpr. II Michael P. Gibson #6353

Badge No.: 6353

Date: 11/16/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01042 **Calib. Date:** 11/16/2011 **Calib. No.:** 00019
Certification File No.: 01043 **Cert. Date:** 11/16/2011 **Cert. No.:** 00013
Linearity File No.: 01044 **Lin. Date:** 11/16/2011 **Lin. No.:** 00013
Solution File No.: 01057 **Soln. Date:** 12/04/2011 **Soln. No.:** 00134
Sequential File No.: 01057 **File Date:** 12/04/2011

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUP S3 0065
Control Solution %: 0.100% **Expires:** 12/16/2012
Solution Control Lot: 10L084 **Bottle No.:** 0382

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:19S		
Control 1 EC	0.100%	20:20S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:21S		
Control 2 EC	0.100%	20:21S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:22S		
Control 3 EC	0.100%	20:22S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:23S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: 21 Joseph Beni

543

Badge No.: 543

Date: 12/04/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01042 Calib. Date: 11/16/2011 Calib. No.: 00019
Certification File No.: 01043 Cert. Date: 11/16/2011 Cert. No.: 00013
Linearity File No.: 01044 Lin. Date: 11/16/2011 Lin. No.: 00013
Solution File No.: 01067 Soln. Date: 12/28/2011 Soln. No.: 00135
Sequential File No.: 01067 File Date: 12/28/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 12/16/2012
Solution Control Lot: 10L084 Bottle No.: 0383

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:46S		
Control 1 EC	0.101%	03:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	03:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:47S		
Control 2 EC	0.099%	03:48S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	03:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:48S		
Control 3 EC	0.099%	03:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	03:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:49S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: Pt 1 / sign L SUM 543

Badge No.: 543

Date: 12/28/2011