

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 01683
Calib. Date: 12/07/2015
Calib. No.: 00031
Certification File No.: 01684
Cert. Date: 12/07/2015
Cert. No.: 00024
Linearity File No.: 01685
Lin. Date: 12/07/2015
Lin. No.: 00024
Solution File No.: 01704
Soln. Date: 01/18/2016
Soln. No.: 00204
Sequential File No.: 01704
File Date: 01/18/2016

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 15H140
Model No.: CU-34
Serial No.: DDUF S3-0065
Expires: 08/04/2017
Bottle No.: 0767

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:51S		
Control 1 EC	0.102%	10:51S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:52S		
Control 2 EC	0.099%	10:53S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:53S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:54S		
Control 3 EC	0.100%	10:54S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:54S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:55S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 01/18/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01683 Calib. Date: 12/07/2015 Calib. No.: 00031
Certification File No.: 01684 Cert. Date: 12/07/2015 Cert. No.: 00024
Linearity File No.: 01685 Lin. Date: 12/07/2015 Lin. No.: 00024
Solution File No.: 01711 Soln. Date: 02/05/2016 Soln. No.: 00205
Sequential File No.: 01711 File Date: 02/05/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 08/04/2017
Solution Control Lot: 15H140 Bottle No.: 0768

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:19S		
Control 1 EC	0.100%	07:20S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	07:20S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:21S		
Control 2 EC	0.098%	07:21S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	07:21S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:22S		
Control 3 EC	0.099%	07:23S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	07:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:24S		

All tests within acceptable tolerance.

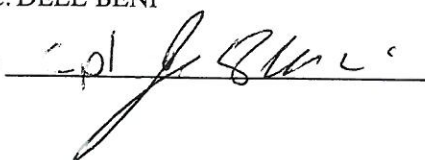
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: 

543

Badge No.: 543

Date: 02/05/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01683 Calib. Date: 12/07/2015 Calib. No.: 00031
Certification File No.: 01684 Cert. Date: 12/07/2015 Cert. No.: 00024
Linearity File No.: 01685 Lin. Date: 12/07/2015 Lin. No.: 00024
Solution File No.: 01718 Soln. Date: 02/20/2016 Soln. No.: 00206
Sequential File No.: 01718 File Date: 02/20/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 08/04/2017
Solution Control Lot: 15H140 Bottle No.: 0769

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	22:32S		
Control 1 EC	0.101%	22:32S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	22:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:33S		
Control 2 EC	0.098%	22:34S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	22:34S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:35S		
Control 3 EC	0.099%	22:35S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	22:35S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:36S		

All tests within acceptable tolerance.

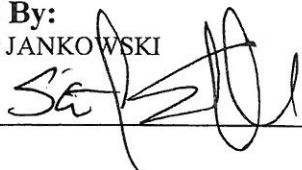
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 02/20/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01683 Calib. Date: 12/07/2015 Calib. No.: 00031
Certification File No.: 01684 Cert. Date: 12/07/2015 Cert. No.: 00024
Linearity File No.: 01685 Lin. Date: 12/07/2015 Lin. No.: 00024
Solution File No.: 01725 Soln. Date: 03/15/2016 Soln. No.: 00207
Sequential File No.: 01725 File Date: 03/15/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 08/04/2017
Solution Control Lot: 15H140 Bottle No.: 0771

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:31S		
Control 1 EC	0.099%	15:32S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:32S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:33S		
Control 2 EC	0.097%	15:33S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:33S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:34S		
Control 3 EC	0.098%	15:35S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:35S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:36S		

All tests within acceptable tolerance.

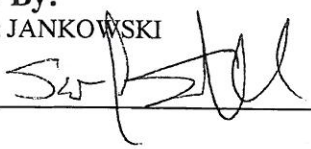
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 03/15/2016

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 01683
Calib. Date: 12/07/2015
Calib. No.: 00031
Certification File No.: 01684
Cert. Date: 12/07/2015
Cert. No.: 00024
Linearity File No.: 01685
Lin. Date: 12/07/2015
Lin. No.: 00024
Solution File No.: 01727
Soln. Date: 04/06/2016
Soln. No.: 00208
Sequential File No.: 01727
File Date: 04/06/2016

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 15H140
Model No.: CU-34
Serial No.: DDUF S3-0065
Expires: 08/04/2017
Bottle No.: 0772

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:19D		
Control 1 EC	0.101%	12:19D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:19D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:20D		
Control 2 EC	0.099%	12:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:22D		
Control 3 EC	0.099%	12:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with
Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #1719

Badge No.: 714

Date: 04/06/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01683 Calib. Date: 12/07/2015 Calib. No.: 00031
Certification File No.: 01684 Cert. Date: 12/07/2015 Cert. No.: 00024
Linearity File No.: 01685 Lin. Date: 12/07/2015 Lin. No.: 00024
Solution File No.: 01736 Soln. Date: 04/18/2016 Soln. No.: 00209
Sequential File No.: 01736 File Date: 04/18/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 08/04/2017
Solution Control Lot: 15H140 Bottle No.: 0773

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:56D		
Control 1 EC	0.100%	13:57D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:57D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:58D		
Control 2 EC	0.098%	13:58D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:59D		
Control 3 EC	0.099%	14:00D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:00D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 04/18/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01738 **Calib. Date:** 04/20/2016 **Calib. No.:** 00032
Certification File No.: 01739 **Cert. Date:** 04/20/2016 **Cert. No.:** 00025
Linearity File No.: 01740 **Lin. Date:** 04/20/2016 **Lin. No.:** 00025
Solution File No.: 01741 **Soln. Date:** 04/20/2016 **Soln. No.:** 00210
Sequential File No.: 01741 **File Date:** 04/20/2016

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0065
Control Solution %: 0.100% **Expires:** 08/04/2017
Solution Control Lot: 15H140 **Bottle No.:** 0774

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:43D		
Control 1 EC	0.102%	13:43D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:43D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:44D		
Control 2 EC	0.101%	13:45D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:45D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:45D		
Control 3 EC	0.101%	13:46D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:46D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDUJPa-144 (MC)

Changed By:

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: Sgt. Michelle L. Goyco

Badge No.: 6040

Date: 04/20/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01738 **Calib. Date:** 04/20/2016 **Calib. No.:** 00032
Certification File No.: 01739 **Cert. Date:** 04/20/2016 **Cert. No.:** 00025
Linearity File No.: 01740 **Lin. Date:** 04/20/2016 **Lin. No.:** 00025
Solution File No.: 01748 **Soln. Date:** 05/09/2016 **Soln. No.:** 00211
Sequential File No.: 01748 **File Date:** 05/09/2016

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0065
Control Solution %: 0.100% **Expires:** 08/04/2017
Solution Control Lot: 15H140 **Bottle No.:** 1201

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:00D		
Control 1 EC	0.100%	11:01D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:01D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:01D		
Control 2 EC	0.099%	11:02D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:02D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:03D		
Control 3 EC	0.100%	11:03D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:03D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:04D		

All tests within acceptable tolerance.

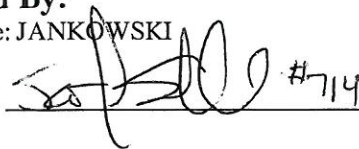
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 05/09/2016

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 01738
Certification File No.: 01739
Linearity File No.: 01740
Solution File No.: 01759
Sequential File No.: 01759
Calib. Date: 04/20/2016
Cert. Date: 04/20/2016
Lin. Date: 04/20/2016
Soln. Date: 06/03/2016
File Date: 06/03/2016
Calib. No.: 00032
Cert. No.: 00025
Lin. No.: 00025
Soln. No.: 00212

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 15H140
Model No.: CU-34
Serial No.: DDUF S3-0065
Expires: 08/04/2017
Bottle No.: 1206

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:46D		
Control 1 EC	0.100%	10:46D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:46D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:47D		
Control 2 EC	0.099%	10:48D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:48D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:48D		
Control 3 EC	0.100%	10:49D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:49D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:50D		

All tests within acceptable tolerance.

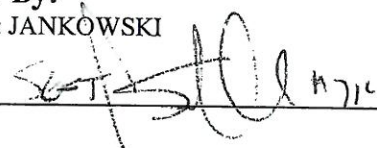
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature: 

Badge No.: 714

Date: 06/03/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01738 **Calib. Date:** 04/20/2016 **Calib. No.:** 00032
Certification File No.: 01739 **Cert. Date:** 04/20/2016 **Cert. No.:** 00025
Linearity File No.: 01740 **Lin. Date:** 04/20/2016 **Lin. No.:** 00025
Solution File No.: 01764 **Soln. Date:** 06/27/2016 **Soln. No.:** 00213
Sequential File No.: 01764 **File Date:** 06/27/2016

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0065
Control Solution %: 0.100% **Expires:** 08/04/2017
Solution Control Lot: 15H140 **Bottle No.:** 1211

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:52D		
Control 1 EC	0.101%	17:52D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	17:52D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:53D		
Control 2 EC	0.099%	17:54D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	17:54D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:54D		
Control 3 EC	0.100%	17:55D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:55D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:56D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 06/27/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01738 Calib. Date: 04/20/2016 Calib. No.: 00032
Certification File No.: 01739 Cert. Date: 04/20/2016 Cert. No.: 00025
Linearity File No.: 01740 Lin. Date: 04/20/2016 Lin. No.: 00025
Solution File No.: 01776 Soln. Date: 07/24/2016 Soln. No.: 00214
Sequential File No.: 01776 File Date: 07/24/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 08/04/2017
Solution Control Lot: 15H140 Bottle No.: 1216

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:51D		
Control 1 EC	-.---%	18:52D	25.4°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	18:52D	25.4°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 07/24/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01738 Calib. Date: 04/20/2016 Calib. No.: 00032
Certification File No.: 01739 Cert. Date: 04/20/2016 Cert. No.: 00025
Linearity File No.: 01740 Lin. Date: 04/20/2016 Lin. No.: 00025
Solution File No.: 01777 Soln. Date: 07/25/2016 Soln. No.: 00215
Sequential File No.: 01777 File Date: 07/25/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 08/04/2017
Solution Control Lot: 15H140 Bottle No.: 1216

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:14D		
Control 1 EC	0.101%	11:14D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	11:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:15D		
Control 2 EC	0.100%	11:15D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:16D		
Control 3 EC	0.100%	11:17D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:17D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 07/25/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01738 Calib. Date: 04/20/2016 Calib. No.: 00032
Certification File No.: 01739 Cert. Date: 04/20/2016 Cert. No.: 00025
Linearity File No.: 01740 Lin. Date: 04/20/2016 Lin. No.: 00025
Solution File No.: 01780 Soln. Date: 08/18/2016 Soln. No.: 00216
Sequential File No.: 01780 File Date: 08/18/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 08/04/2017
Solution Control Lot: 15H140 Bottle No.: 1221

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:53D		
Control 1 EC	0.101%	15:54D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:55D		
Control 2 EC	0.100%	15:55D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	15:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:56D		
Control 3 EC	0.100%	15:56D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	15:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:57D		

All tests within acceptable tolerance.

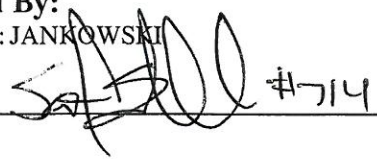
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 08/18/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01738 Calib. Date: 04/20/2016 Calib. No.: 00032
Certification File No.: 01739 Cert. Date: 04/20/2016 Cert. No.: 00025
Linearity File No.: 01740 Lin. Date: 04/20/2016 Lin. No.: 00025
Solution File No.: 01790 Soln. Date: 09/15/2016 Soln. No.: 00217
Sequential File No.: 01790 File Date: 09/15/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 05/17/2018
Solution Control Lot: 201605D Bottle No.: 1303

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:03D		
Control 1 EC	0.100%	20:03D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	20:03D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:04D		
Control 2 EC	0.100%	20:04D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	20:04D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:05D		
Control 3 EC	0.100%	20:06D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	20:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:06D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: cp1 J 8m4 543

Badge No.: 543

Date: 09/15/2016

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 01738
Calib. Date: 04/20/2016
Calib. No.: 00032
Certification File No.: 01739
Cert. Date: 04/20/2016
Cert. No.: 00025
Linearity File No.: 01740
Lin. Date: 04/20/2016
Lin. No.: 00025
Solution File No.: 01797
Soln. Date: 10/14/2016
Soln. No.: 00218
Sequential File No.: 01797
File Date: 10/14/2016

Calibrating Unit: WET
Model No.: CU-34
Serial No.: DDUF S3-0065
Control Solution %: 0.100%
Expires: 05/17/2018
Solution Control Lot: 201605D
Bottle No.: 1304

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	02:26D		
Control 1 EC	0.101%	02:27D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.103%	02:27D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:27D		
Control 2 EC	0.101%	02:28D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	02:28D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:29D		
Control 3 EC	0.101%	02:29D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	02:29D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:30D		

All tests within acceptable tolerance.

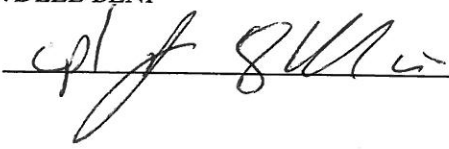
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: 

Badge No.: 543

Date: 10/14/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01798 **Calib. Date:** 10/17/2016 **Calib. No.:** 00033
Certification File No.: 01799 **Cert. Date:** 10/17/2016 **Cert. No.:** 00026
Linearity File No.: 01800 **Lin. Date:** 10/17/2016 **Lin. No.:** 00026
Solution File No.: 01801 **Soln. Date:** 10/17/2016 **Soln. No.:** 00219
Sequential File No.: 01801 **File Date:** 10/17/2016

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 05/17/2018
Solution Control Lot: 201605D **Bottle No.:** 1305

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:06D		
Control 1 EC	0.102%	16:06D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	16:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:07D		
Control 2 EC	0.101%	16:07D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	16:07D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:08D		
Control 3 EC	0.101%	16:09D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	16:09D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:09D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with
Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDSFp2 - 0396 (MA)

Changed By:

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: Sgt. Michelle Delo #6040

Badge No.: 6040

Date: 10/17/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01798 Calib. Date: 10/17/2016 Calib. No.: 00033
Certification File No.: 01799 Cert. Date: 10/17/2016 Cert. No.: 00026
Linearity File No.: 01800 Lin. Date: 10/17/2016 Lin. No.: 00026
Solution File No.: 01808 Soln. Date: 11/19/2016 Soln. No.: 00220
Sequential File No.: 01808 File Date: 11/19/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 05/17/2018
Solution Control Lot: 201605D Bottle No.: 1306

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:01S		
Control 1 EC	0.101%	18:02S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:02S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:03S		
Control 2 EC	0.100%	18:03S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	18:03S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:04S		
Control 3 EC	0.101%	18:05S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:05S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:05S		

All tests within acceptable tolerance.

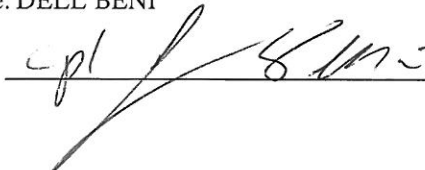
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: 

Badge No.: 543

Date: 11/19/2016

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 01798
Calib. Date: 10/17/2016
Calib. No.: 00033
Certification File No.: 01799
Cert. Date: 10/17/2016
Cert. No.: 00026
Linearity File No.: 01800
Lin. Date: 10/17/2016
Lin. No.: 00026
Solution File No.: 01814
Soln. Date: 12/26/2016
Soln. No.: 00221
Sequential File No.: 01814
File Date: 12/26/2016

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 201605D
Model No.: CU-34
Serial No.: DDUF S3-0064
Expires: 05/17/2018
Bottle No.: 1308

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:16S		
Control 1 EC	0.101%	07:17S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	07:17S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:17S		
Control 2 EC	0.100%	07:18S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	07:18S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:19S		
Control 3 EC	0.101%	07:19S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	07:19S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:20S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JANKOWSKI

First Name: JOSEPH

MI: E

Signature:  #714

Badge No.: 714

Date: 12/26/2016