

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01798 Calib. Date: 10/17/2016 Calib. No.: 00033
Certification File No.: 01799 Cert. Date: 10/17/2016 Cert. No.: 00026
Linearity File No.: 01800 Lin. Date: 10/17/2016 Lin. No.: 00026
Solution File No.: 01818 Soln. Date: 01/23/2017 Soln. No.: 00222
Sequential File No.: 01818 File Date: 01/23/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 05/17/2018
Solution Control Lot: 201605D Bottle No.: 1307

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:49S		
Control 1 EC	0.101%	14:50S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:50S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:51S		
Control 2 EC	0.099%	14:51S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	14:51S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:52S		
Control 3 EC	0.099%	14:53S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	14:53S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:53S		

All tests within acceptable tolerance.

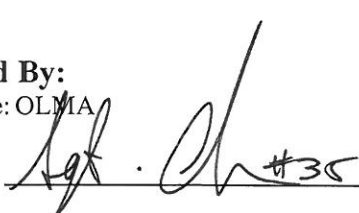
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature:  #35

Badge No.: 735

Date: 01/23/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01798 **Calib. Date:** 10/17/2016 **Calib. No.:** 00033
Certification File No.: 01799 **Cert. Date:** 10/17/2016 **Cert. No.:** 00026
Linearity File No.: 01800 **Lin. Date:** 10/17/2016 **Lin. No.:** 00026
Solution File No.: 01822 **Soln. Date:** 02/10/2017 **Soln. No.:** 00223
Sequential File No.: 01822 **File Date:** 02/10/2017

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 12/02/2018
Solution Control Lot: 16390 **Bottle No.:** 1366

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:46S		
Control 1 EC	0.101%	13:46S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:46S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:47S		
Control 2 EC	0.099%	13:48S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:48S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:49S		
Control 3 EC	0.099%	13:49S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:49S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:50S		

All tests within acceptable tolerance.

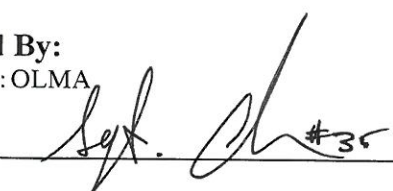
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature: 

Badge No.: 735

Date: 02/10/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01798 Calib. Date: 10/17/2016 Calib. No.: 00033
Certification File No.: 01799 Cert. Date: 10/17/2016 Cert. No.: 00026
Linearity File No.: 01800 Lin. Date: 10/17/2016 Lin. No.: 00026
Solution File No.: 01828 Soln. Date: 03/03/2017 Soln. No.: 00224
Sequential File No.: 01828 File Date: 03/03/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 12/02/2018
Solution Control Lot: 16390 Bottle No.: 1382

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:35S		
Control 1 EC	0.100%	13:35S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	13:35S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:36S		
Control 2 EC	0.098%	13:37S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	13:37S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:37S		
Control 3 EC	0.099%	13:38S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:38S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:39S		

All tests within acceptable tolerance.

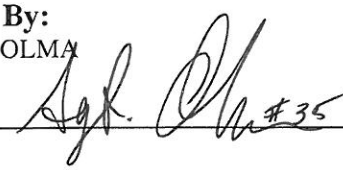
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature: 

Badge No.: 735

Date: 03/03/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01829 Calib. Date: 03/06/2017 Calib. No.: 00034
Certification File No.: 01830 Cert. Date: 03/06/2017 Cert. No.: 00027
Linearity File No.: 01831 Lin. Date: 03/06/2017 Lin. No.: 00027
Solution File No.: 01834 Soln. Date: 03/24/2017 Soln. No.: 00226
Sequential File No.: 01834 File Date: 03/24/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 12/02/2018
Solution Control Lot: 16390 Bottle No.: 1403

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:43S		
Control 1 EC	0.104%	09:43S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:43S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:44S		
Control 2 EC	0.101%	09:45S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	09:45S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:46S		
Control 3 EC	0.101%	09:46S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	09:46S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:47S		

All tests within acceptable tolerance.

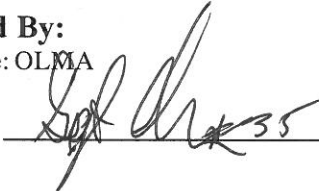
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature: 

Badge No.: 735

Date: 03/24/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01829 **Calib. Date:** 03/06/2017 **Calib. No.:** 00034
Certification File No.: 01830 **Cert. Date:** 03/06/2017 **Cert. No.:** 00027
Linearity File No.: 01831 **Lin. Date:** 03/06/2017 **Lin. No.:** 00027
Solution File No.: 01836 **Soln. Date:** 04/14/2017 **Soln. No.:** 00227
Sequential File No.: 01836 **File Date:** 04/14/2017

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 12/02/2018
Solution Control Lot: 16390 **Bottle No.:** 1373

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:34D		
Control 1 EC	0.103%	11:35D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.103%	11:35D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:35D		
Control 2 EC	0.101%	11:36D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	11:36D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:37D		
Control 3 EC	0.101%	11:37D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	11:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature:  #35

Badge No.: 735

Date: 04/14/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01829 Calib. Date: 03/06/2017 Calib. No.: 00034
Certification File No.: 01830 Cert. Date: 03/06/2017 Cert. No.: 00027
Linearity File No.: 01831 Lin. Date: 03/06/2017 Lin. No.: 00027
Solution File No.: 01844 Soln. Date: 05/07/2017 Soln. No.: 00228
Sequential File No.: 01844 File Date: 05/07/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 12/02/2018
Solution Control Lot: 16390 Bottle No.: 1345

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:16D		
Control 1 EC	0.102%	09:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	09:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:17D		
Control 2 EC	0.101%	09:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	09:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:18D		
Control 3 EC	0.102%	09:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.104%	09:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature: _____

Badge No.: 735

Date: 05/07/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01829 Calib. Date: 03/06/2017 Calib. No.: 00034
Certification File No.: 01830 Cert. Date: 03/06/2017 Cert. No.: 00027
Linearity File No.: 01831 Lin. Date: 03/06/2017 Lin. No.: 00027
Solution File No.: 01851 Soln. Date: 05/26/2017 Soln. No.: 00229
Sequential File No.: 01851 File Date: 05/26/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 01/30/2019
Solution Control Lot: 17050 Bottle No.: 0260

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:14D		
Control 1 EC	0.104%	12:15D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	12:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:16D		
Control 2 EC	0.102%	12:16D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	12:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:17D		
Control 3 EC	0.102%	12:18D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	12:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:18D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature: 

Badge No.: 735

Date: 05/26/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01829 Calib. Date: 03/06/2017 Calib. No.: 00034
Certification File No.: 01830 Cert. Date: 03/06/2017 Cert. No.: 00027
Linearity File No.: 01831 Lin. Date: 03/06/2017 Lin. No.: 00027
Solution File No.: 01855 Soln. Date: 06/15/2017 Soln. No.: 00230
Sequential File No.: 01855 File Date: 06/15/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 01/30/2019
Solution Control Lot: 17050 Bottle No.: 0446

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:50D		
Control 1 EC	0.102%	13:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	13:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:51D		
Control 2 EC	0.101%	13:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	13:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:53D		
Control 3 EC	0.101%	13:53D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:53D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:54D		

All tests within acceptable tolerance.

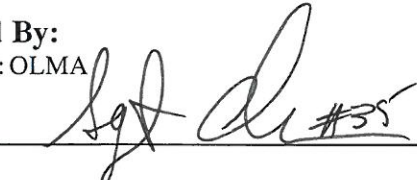
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature: 

Badge No.: 735

Date: 06/15/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01829 Calib. Date: 03/06/2017 Calib. No.: 00034
Certification File No.: 01830 Cert. Date: 03/06/2017 Cert. No.: 00027
Linearity File No.: 01831 Lin. Date: 03/06/2017 Lin. No.: 00027
Solution File No.: 01864 Soln. Date: 07/07/2017 Soln. No.: 00231
Sequential File No.: 01864 File Date: 07/07/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064
Control Solution %: 0.100% Expires: 01/30/2019
Solution Control Lot: 17050 Bottle No.: 0418

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:32D		
Control 1 EC	-.---%	13:33D	24.4°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	13:33D	24.4°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

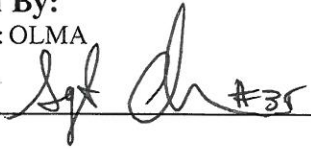
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature: 

Badge No.: 735

Date: 07/07/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0005
Location:	PLAINSBORO TOWNSHIP PD		
Calibration File No.:	01829	Calib. Date:	03/06/2017
Certification File No.:	01830	Cert. Date:	03/06/2017
Linearity File No.:	01831	Lin. Date:	03/06/2017
Solution File No.:	01865	Soln. Date:	07/09/2017
Sequential File No.:	01865	File Date:	07/09/2017
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUF S3-0064
Solution Control Lot:	17050	Expires:	01/30/2019
		Bottle No.:	0398

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:00D		
Control 1 EC	0.103%	04:00D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	04:00D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:01D		
Control 2 EC	0.102%	04:02D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	04:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:02D		
Control 3 EC	0.102%	04:03D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	04:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:04D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature: 

Badge No.: 735

Date: 07/09/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01829 **Calib. Date:** 03/06/2017 **Calib. No.:** 00034
Certification File No.: 01830 **Cert. Date:** 03/06/2017 **Cert. No.:** 00027
Linearity File No.: 01831 **Lin. Date:** 03/06/2017 **Lin. No.:** 00027
Solution File No.: 01872 **Soln. Date:** 07/28/2017 **Soln. No.:** 00233
Sequential File No.: 01872 **File Date:** 07/28/2017

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0064
Control Solution %: 0.100% **Expires:** 01/30/2019
Solution Control Lot: 17050 **Bottle No.:** 0474

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:57D		
Control 1 EC	0.101%	10:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	10:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:59D		
Control 2 EC	0.101%	10:59D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.104%	10:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:00D		
Control 3 EC	0.101%	11:00D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	11:00D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:01D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature: 

Badge No.: 735

Date: 07/28/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0005
Location:	PLAINSBORO TOWNSHIP PD		
Calibration File No.:	01829	Calib. Date:	03/06/2017
Certification File No.:	01830	Cert. No.:	00034
Linearity File No.:	01831	Cert. Date:	03/06/2017
Solution File No.:	01876	Lin. Date:	03/06/2017
Sequential File No.:	01876	Soln. Date:	08/18/2017
		File Date:	08/18/2017
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUF S3-0064
Solution Control Lot:	17050	Expires:	01/30/2019
		Bottle No.:	0443

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:51D		
Control 1 EC	0.102%	12:51D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	12:51D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:52D		
Control 2 EC	0.101%	12:53D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	12:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:53D		
Control 3 EC	0.102%	12:54D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	12:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:55D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

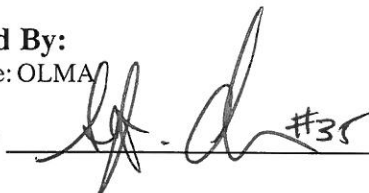
Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature:

 #35

Badge No.: 735

Date: 08/18/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01879 **Calib. Date:** 08/23/2017 **Calib. No.:** 00035
Certification File No.: 01880 **Cert. Date:** 08/23/2017 **Cert. No.:** 00028
Linearity File No.: 01881 **Lin. Date:** 08/23/2017 **Lin. No.:** 00028
Solution File No.: 01882 **Soln. Date:** 08/23/2017 **Soln. No.:** 00235
Sequential File No.: 01882 **File Date:** 08/23/2017

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0065
Control Solution %: 0.100% **Expires:** 06/28/2019
Solution Control Lot: 17200 **Bottle No.:** 1438

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:22D		
Control 1 EC	0.099%	11:23D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	11:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:23D		
Control 2 EC	0.098%	11:24D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:25D		
Control 3 EC	0.098%	11:25D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:26D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DD VJP 2-144 (DR)

Changed By:

Last Name: KLIMIK

First Name: DAVID

MI: W

Signature: T. P. D. Klimik # 7040

Badge No.: 7040

Date: 08/23/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01879 **Calib. Date:** 08/23/2017 **Calib. No.:** 00035
Certification File No.: 01880 **Cert. Date:** 08/23/2017 **Cert. No.:** 00028
Linearity File No.: 01881 **Lin. Date:** 08/23/2017 **Lin. No.:** 00028
Solution File No.: 01892 **Soln. Date:** 09/26/2017 **Soln. No.:** 00236
Sequential File No.: 01892 **File Date:** 09/26/2017

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0065
Control Solution %: 0.100% **Expires:** 06/28/2019
Solution Control Lot: 17200 **Bottle No.:** 1431

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:12D		
Control 1 EC	0.100%	10:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:13D		
Control 2 EC	0.099%	10:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:14D		
Control 3 EC	0.100%	10:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:15D		

All tests within acceptable tolerance.

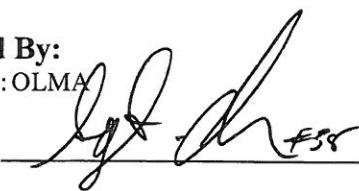
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature: 

Badge No.: 735

Date: 09/26/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01879 **Calib. Date:** 08/23/2017 **Calib. No.:** 00035
Certification File No.: 01880 **Cert. Date:** 08/23/2017 **Cert. No.:** 00028
Linearity File No.: 01881 **Lin. Date:** 08/23/2017 **Lin. No.:** 00028
Solution File No.: 01896 **Soln. Date:** 10/13/2017 **Soln. No.:** 00237
Sequential File No.: 01896 **File Date:** 10/13/2017

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUF S3-0065
Control Solution %: 0.100% **Expires:** 06/28/2019
Solution Control Lot: 17200 **Bottle No.:** 1461

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:28D		
Control 1 EC	0.099%	12:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:29D		
Control 2 EC	0.098%	12:30D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:30D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:30D		
Control 3 EC	0.099%	12:31D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:31D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:32D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMAN

First Name: BRETT

MI: J

Signature:  #35

Badge No.: 735

Date: 10/13/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01879 Calib. Date: 08/23/2017 Calib. No.: 00035
Certification File No.: 01880 Cert. Date: 08/23/2017 Cert. No.: 00028
Linearity File No.: 01881 Lin. Date: 08/23/2017 Lin. No.: 00028
Solution File No.: 01901 Soln. Date: 11/04/2017 Soln. No.: 00238
Sequential File No.: 01901 File Date: 11/04/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 06/28/2019
Solution Control Lot: 17200 Bottle No.: 1409

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:03S		
Control 1 EC	0.100%	06:04S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	06:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:04S		
Control 2 EC	0.099%	06:05S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	06:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:06S		
Control 3 EC	0.100%	06:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	06:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: _____

Badge No.: 543

Date: 11/04/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01879 Calib. Date: 08/23/2017 Calib. No.: 00035
Certification File No.: 01880 Cert. Date: 08/23/2017 Cert. No.: 00028
Linearity File No.: 01881 Lin. Date: 08/23/2017 Lin. No.: 00028
Solution File No.: 01911 Soln. Date: 11/27/2017 Soln. No.: 00239
Sequential File No.: 01911 File Date: 11/27/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 06/28/2019
Solution Control Lot: 17200 Bottle No.: 1444

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:15S		
Control 1 EC	0.100%	15:16S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:17S		
Control 2 EC	0.098%	15:17S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:18S		
Control 3 EC	0.099%	15:19S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:19S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OLMA

First Name: BRETT

MI: J

Signature: _____

Badge No.: 735

Date: 11/27/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01879 Calib. Date: 08/23/2017 Calib. No.: 00035
Certification File No.: 01880 Cert. Date: 08/23/2017 Cert. No.: 00028
Linearity File No.: 01881 Lin. Date: 08/23/2017 Lin. No.: 00028
Solution File No.: 01920 Soln. Date: 12/26/2017 Soln. No.: 00240
Sequential File No.: 01920 File Date: 12/26/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 06/28/2019
Solution Control Lot: 17200 Bottle No.: 0669

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:31S		
Control 1 EC	0.099%	20:31S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:32S		
Control 2 EC	0.098%	20:33S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:34S		
Control 3 EC	0.098%	20:34S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:35S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELL BENI

First Name: JOSEPH

MI: M

Signature: Cpl J. Beni 543

Badge No.: 543

Date: 12/26/2017